

# Blood Pressure Sensor

(Order Code BPS-BTA)The Vernier Blood



Pressure Sensor is used to measure systemic arterial blood pressure in humans (non-invasively). When used with Logger Pro<sup>®</sup> 3.4 or newer, Logger Lite<sup>®</sup> 1.3.1 or newer, or LabQuest App 1.2 or newer, it can measure arterial blood pressure and calculate both the systolic and diastolic blood pressure using the oscillometric method.

The following is a partial list of activities and experiments that can be performed using this sensor.

- Measure blood pressure before and after exercise.
- Measure blood pressure while sitting or standing.
- Compare blood pressure after voluntary isometric contractions (weight lifting) and a rhythmic activity such as running or biking.
- Investigate how digestion affects blood pressure.
- Study the effect of caffeine on blood pressure.
- Compare blood pressure between smokers and non-smokers.

## What is included with the Blood Pressure Sensor?

- Blood Pressure Sensor
- Standard adult size adjustable cuff (27 cm to 39 cm)
- Bulb pump (with release valve)
- Blood Pressure Sensor booklet (this booklet)

## How the Blood Pressure Sensor Works

The active sensor in this unit is the SenSym SDX05D4 pressure transducer. It has a membrane which flexes as pressure changes. This sensor is arranged to measure differential pressure. The sensor produces an output voltage which varies with the pressure measured in the cuff. It includes special circuitry to minimize errors caused by changes in temperature. We provide an amplifier circuit that conditions the signal from the pressure transducer. With this circuit, the output voltage from the Blood Pressure Sensor will be linear with respect to pressure.

This sensor is equipped with circuitry that supports auto-ID. When used with LabQuest, LabQuest Mini, LabPro, Go! Link, or SensorDAQ, the data-collection software identifies the sensor and uses pre-defined parameters to configure an experiment appropriate to the recognized sensor.

## Collecting Data with the Blood Pressure Sensor

This sensor can be used with the following interfaces to collect data:

- Vernier LabQuest<sup>®</sup> as a standalone device or with a computer
- Vernier LabQuest<sup>®</sup> Mini with a computer
- Vernier LabPro<sup>®</sup> with a computer
- Vernier Go!<sup>®</sup>Link
- Vernier SensorDAQ<sup>™</sup>

The Blood Pressure Sensor is not compatible with TI calculators for data collection.

Here is the general procedure to follow when using the Blood Pressure Sensor:

1. Connect the Blood Pressure Sensor to the interface.
2. Start the data-collection software.
3. The software will identify the Blood Pressure Sensor and load a default data-collection setup. You are now ready to collect data.

## Data-Collection Software

This sensor can be used with an interface and the following data-collection software.

- **Logger Pro** This computer program is used with LabQuest, LabQuest Mini, LabPro, or Go!Link.
- **Logger Lite** This computer program is used with LabQuest, LabQuest Mini, LabPro, or Go!Link.
- **LabVIEW** National Instruments LabVIEW<sup>™</sup> software is a graphical programming language sold by National Instruments. It is used with SensorDAQ and can be used with a number of other Vernier interfaces. See [www.vernier.com/labview](http://www.vernier.com/labview) for more information.

**NOTE:** This product is to be used for educational purposes only. It is not appropriate for industrial, medical, research, or commercial applications.


## Using the Blood Pressure Sensor with a Computer

When performing blood pressure measurements, it is best to work with a partner.

Currently, Logger Lite only supports blood pressure measurements in mm Hg.

Follow these general procedures to use the Blood Pressure Sensor with a computer:

1. Connect the Blood Pressure Sensor to Channel 1 on the LabPro, LabQuest, LabQuest Mini, or to a Go!Link connected to a computer. Attach the rubber hose from the cuff to the connector on the sensor.
2. Wrap the cuff firmly around your partner's arm, approximately 2 cm above the elbow. The two rubber hoses from the cuff should be positioned over the bicep muscle (brachial artery) and not under the arm. **Important:** *The person having his or her blood pressure measured must remain still during data collection—no movement of the arm or hand during measurements.*
3. Start Logger Pro (version 3.4 or newer) or Logger Lite (version 1.3 or newer) on the computer.

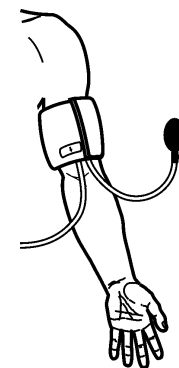


4. Logger *Pro* or Logger *Lite* will identify the Blood Pressure Sensor and load the proper calibration. You are now ready to collect data.
5. Click **Collect** to begin collecting data.
6. Quickly and repeatedly squeeze the bulb to inflate the cuff on your partner's arm. Continue inflating the cuff to a pressure between 150 and 170 mm Hg. A meter in the data-collection software will display the live pressure readings from the sensor. When the maximum pressure is reached, set the bulb pump down onto the table. The built-in pressure release valve will slowly deflate the cuff.
7. After the pressure drops to 50 mm Hg, click **Stop** in the data-collection software and press down on the pressure release valve to release any air left in the cuff. If the pressure does not reach 50 mm Hg by the time data collection ends, adjust the exhaust rate of the pressure release valve according to the directions listed under "Adjusting the Pressure Release Valve".

### Using the Blood Pressure Sensor with LabQuest (standalone)

When performing blood pressure measurements, it is best to work with a partner. Follow these general procedures to use the Blood Pressure Sensor with LabQuest as a standalone device.

1. Connect the Blood Pressure Sensor to LabQuest. Attach the rubber hose from the cuff to the connector on the sensor.
2. Wrap the cuff firmly around your partner's arm, approximately 2 cm above the elbow. The two rubber hoses from the cuff should be positioned over the bicep muscle (brachial artery) and not under the arm. **Important:** *The person having his or her blood pressure measured must remain still during data collection—no movement of the arm or hand during measurements.*
3. LabQuest App will identify the Blood Pressure Sensor and load the proper calibration. You are now ready to collect data.
4. Start data collection.
5. Quickly and repeatedly squeeze the bulb to inflate the cuff on your partner's arm. Continue inflating the cuff to a pressure between 150 and 170 mm Hg. A meter in the data-collection software will display the live pressure readings from the sensor. When the maximum pressure is reached, set the bulb pump down onto the table. The built-in pressure release valve will slowly deflate the cuff.
6. After the pressure drops to 50 mm Hg, stop data collection and press down on the pressure release valve to release any air left in the cuff. If the pressure does not reach 50 mm Hg by the time data collection ends, adjust the exhaust rate of the pressure release valve according to the directions listed under "Adjusting the Pressure Release Valve".

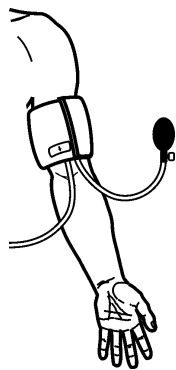

### Helpful Tips

Blood pressure readings will differ from person to person and even between measurements on the same individual. Do not expect to receive the same measurements each trial since there are many factors that cause a person's blood pressure to increase or decrease. Use the following tips to take accurate measurements.

- The subject's arm and hand must remain still during measurements.
- Proper placement of the pressure cuff will increase the accuracy of your blood pressure measurements. The rubber hoses from the cuff should exit over the brachial artery and 2 cm above the crease in the elbow.
- Accurate blood pressure readings depend on the use of a cuff of appropriate size for the arm. For younger students, a smaller cuff is available (18 cm to 27 cm). Our small blood pressure cuff can be ordered separately: order code CUFF-SM. A large cuff is also available for students with arm circumferences greater than 39 cm: order code CUFF-LG.
- Do not touch or move the exhaust valve during measurements.
- Remove any clothing that may cover or constrict the portion of the arm being measured.
- For most individuals it is not necessary to inflate the pressure cuff higher than 170 mm Hg. Over inflation of the cuff may cause pain and/or injury.
- If the pressure release valve is exhausting slower or faster than 2.0–4.0 mmHg/s, then adjust the exhaust rate of the pressure valve.


### Blood Pressure Sensor Specifications

#### Calibration

Slope	56.11 (mm Hg/V)
Intercept	0.00 (mm Hg)
Pressure range	0 mm Hg to 250 mm Hg
Maximum pressure without permanent damage	1030 mm Hg
Typical accuracy	± 3 mm Hg
Temperature Compensated	0°C to 50°C
Sensing element	SenSym SDX05D4
Combined linearity and hysteresis	typical ±0.2% full scale
Response time	100 microseconds

### Adjusting the Pressure Release Valve


The pressure release valve is set to release at a rate of 3.0 mm Hg/second on an arm of 32 cm in circumference. For arms much larger or much smaller it may be necessary to adjust the valve so that the exhaust rate stays in the range of 2.0–4.0 mmHg/s. With the bulb in hand and the hose leading away from you, place a screwdriver into the metal slot on the top of the release valve. To increase the rate of exhaust, turn the screwdriver clockwise. To decrease the rate of exhaust, turn the screwdriver counter-clockwise. The larger a subject's arm the slower the release valve will exhaust.



## Calculating Blood Pressure (Oscillometric Method)


The oscillometric method is a non-invasive means of measuring blood pressure. It is based on the principle that blood pumped through the arteries by the heart causes the arterial walls to flex. When a cuff (placed around the upper arm to occlude the brachial artery) is inflated and then slowly deflated at a constant rate, an arterial pressure pulse forms. These pressure pulses pass from the arteries, through the arm, and into the pressure cuff itself.

When the artery is fully compressed, blood flow stops along with the pulsations. As the pressure in the cuff is slowly decreased, the arterial blood pressure increases to the point that blood is forced through the artery in short pulses. As the pressure in the cuff continues to decrease, more blood flows through the occluded artery and the pulses become increasingly significant until maximum amplitude is reached. Further decrease of the cuff pressure minimizes the occlusion of the artery and the pulses continue to decrease until the occlusion is removed.

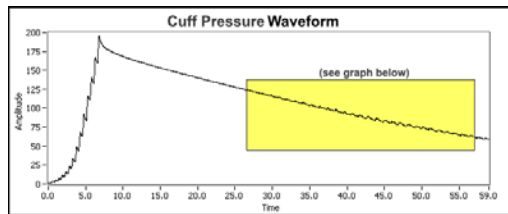

*Cuff pressure measured by sensor*

These pressure pulses, when separated from the decaying mean pressure of the cuff, form an oscillating waveform (see figure below). The peak-to-peak amplitudes of this waveform create a bell shaped "envelope". Within the envelope, the amplitudes of the waveform increase through the systolic blood pressure and continue increasing until the mean arterial pressure (MAP) is reached. Physiologically, the cuff pressure corresponding to the maximum amplitude approximates the mean arterial pressure. Generally, the systolic blood pressure is calculated by determining the point along the envelope prior to the MAP using a known percentage of the maximum amplitude. Diastolic blood pressure is calculated using the same method and the portion of the envelope following the MAP.

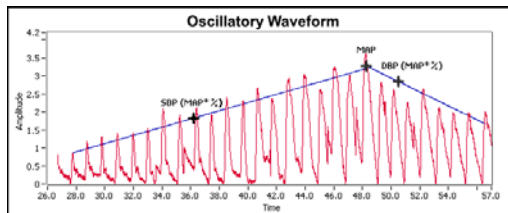


*Oscillatory waveform used to create "Envelope"*

## Using the BPS at high altitudes (above 6,000 ft)

To record proper measurements at altitudes above 6,000 ft (0.8 atm or 609 mm/Hg) the pressure release valve will need to be readjusted. The pressure release valve is set to release at a rate of 3.0 mmHg/s at sea level, where atmospheric pressure is 1 atm or 760 mm/Hg. At higher altitudes, the pressure release valve will exhaust at a slower rate. To use the Blood Pressure Sensor at Altitudes above 6,000 ft, open the pressure exhaust valve by turning it a half turn clockwise. See the instructions above. Verify that the exhaust rate is now in the range of 2.0–4.0 mmHg/s after making the adjustment.

## Warranty

Vernier warrants this product to be free from defects in materials and workmanship for a period of five years from the date of shipment to the customer. This warranty does not cover damage to the product caused by abuse or improper use.

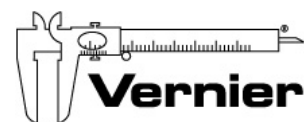

**Measure. Analyze. Learn.™**

**Vernier Software & Technology**

13979 S.W. Millikan Way • Beaverton, OR 97005-2886

Toll Free (888) 837-6437 • (503) 277-2299 • FAX (503) 277-2440

info@vernier.com • www.vernier.com

Rev.8/2/11

Logger *Pro*, Logger Lite, Vernier LabQuest, Vernier LabQuest Mini, Vernier LabPro, Go! Link, Vernier EasyLink and other marks shown are our trademarks or registered trademarks in the United States.

CBL 2 and CBL, TI-GRAPH LINK, and TI Connect are trademarks of Texas Instruments.

All other marks not owned by us that appear herein are the property of their respective owners, who may or may not be affiliated with, connected to, or sponsored by us.



Printed on recycled paper.